

Sample Received: February 16, 2026

COA Issued: February 19, 2026

PRODUCT INFORMATION

Vendor: **BioSync Solutions** **Sample Name:** **Glow Blend 10/10/50mg** **Sample Type:** **Blue lyophilized powder** **Lot Number:** **25051**

MW
1419.5, 4964.1 , & 403.4 g/mol

ANALYTICAL METHODS

Identity: Confirmed via MALDI—MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation


TEST RESULTS

Specification	Result	Method	
Identity: BPC-157, TB-500 & GHK-Cu	BPC—157, TB—500 & GHK-Cu	MALDI—MS	✓ Conforms
Content	10.12, 9.95 & 50.23 mg	HPLC Quantitation	✓ Conforms
Purity	99.8%	RP-HPLC (214 nm)	✓ Conforms



ANALYTICAL DATA

HPLC Chromatogram (Retention Time: 5.7, 5.9 & 2.092 min)

<https://biosyncsolutions.store/>

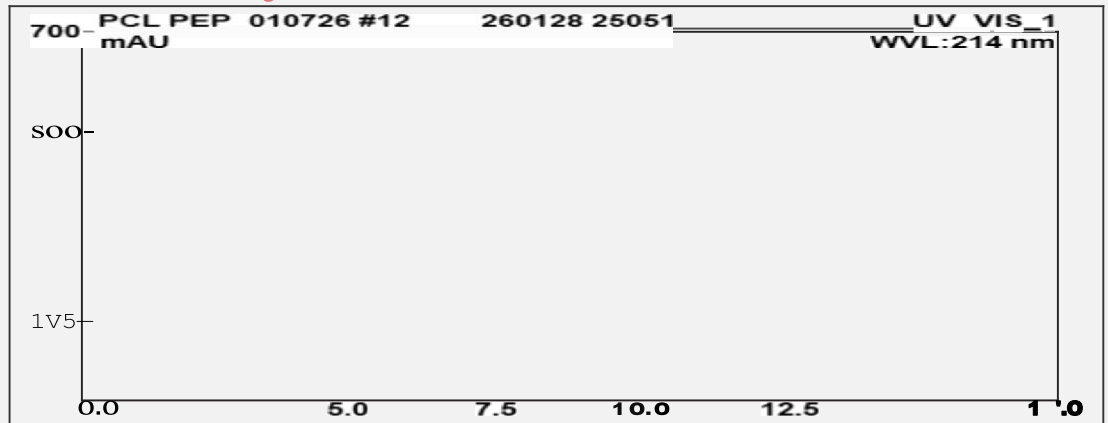

Mass Spectrum (MALDI-MS)

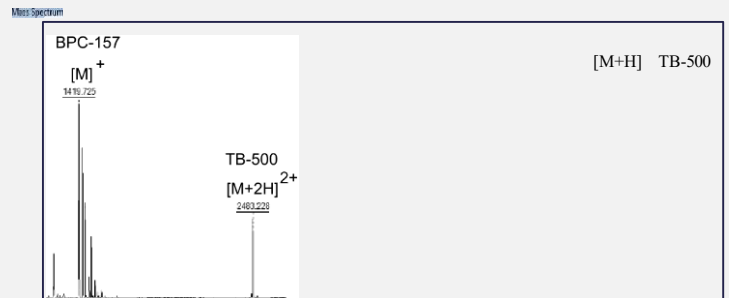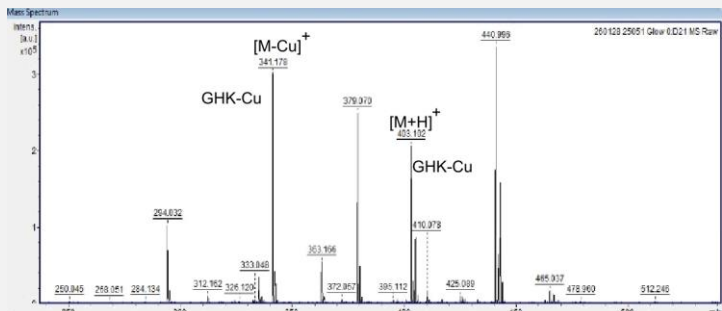

Certification: This COA confirms that the tested material meets or exceeds Bio Gen Lab's analytical quality specifications for peptide research use.

Visit: <https://biogenlab.org>.

Shane Straight
Shane Straight, M.S.
Principal Chemist, Bio Gen Lab